

Copy Control 15 Red FISH Probe

Control Number: 901-7217-071817

BIOCARE
M E D I C A L

Catalog Number: PFI7217V
Description: Copy Control 15 Red FISH Probe
Dilution: Ready-to-use
Volume: 25 µL



Intended Use:
For In Vitro Diagnostic Use.

Copy Control 15 Red FISH Probe is designed to hybridize to human α -satellite DNA sequences located at the centromere region of chromosome 15. The clinical interpretation of any positive or negative hybridization events should be complemented by the use of appropriate controls and other diagnostic tests where appropriate. Evaluation should be carried out within the context of the patient's clinical history by a qualified pathologist.

FOR DISTRIBUTION OUTSIDE THE UNITED STATES ONLY

Summary and Explanation:

Biocare Medical Copy Control probes are designed to serve as enumeration probes for a variety of FISH assays. The Copy Control 15 Probe provides coverage of the 15p11.1-q11.1 region of chromosome 15.

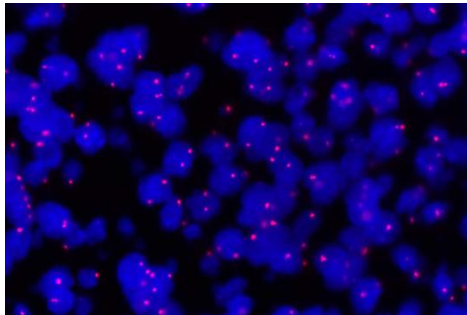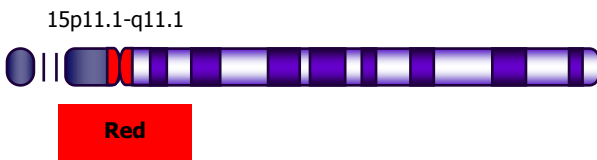


Copy Control 15 Red FISH probe hybridized on FFPE tissue.

Principle of Procedure:

Fluorescent in situ hybridization (FISH) is used to detect specific sequences of chromosomal DNA by using probes, or short fragments, of complementary DNA that have been fluorescently labeled. The hybridization between the probe and its target DNA sequence can be detected under a fluorescent microscope.

Species Reactivity: Human

 Biocare Medical
60 Berry Drive
Pacheco, CA 94553
USA



Rev: 062117

Tel: 800-799-9499 | www.biocare.net | Fax: 925-603-8080

Known Application:

Fluorescence In-Situ Hybridization (FISH) on formalin-fixed paraffin embedded (FFPE) tissues.

Supplied As: Probe in hybridization buffer.

Storage and Stability:

Store probe at -20°C and away from light. The product is stable to the expiration date printed on the label, when stored under these conditions. Do not use after expiration date.

Protocol Recommendations:

1. Add 2.5 µl of probe to 7.5 µl of FISH Hybridization Buffer (FRR7311A), mix well and briefly centrifuge.
2. Apply 10 µl of probe mix to the selected target area of the slide.
3. Cover with an 18 mm x 18 mm cover glass and seal with rubber cement.
4. Place sealed slide on thermal cycler designed to perform denaturation and hybridization steps in slide-based FISH procedures (please see manufacturer's operating instructions).
5. Denature probe at 83°C for 5 minutes and hybridize at 37°C between 12-18 hours.
6. Remove cover glass and wash slides using the following conditions:
 - 6.1. Wash 1: 2x SSC/0.3% Nonident-P40 at 72°C±1°C for 2 minutes
 - 6.2. Wash 2: 2x SSC/0.1% Nonident-P40 at room temperature for 2 minutes
7. Apply 10 µl of a DAPI nuclear counterstain directly to the target area of the slide; cover area using a 24 mm x 50 mm cover glass.
8. Slides are ready for visualization using a fluorescent microscope.

Technical Note:

Biocare Medical FISH probes are optimized to provide the best signal performance using optical filters that can accommodate the excitation/emission wavelengths specified below. Using filters outside these spectral specifications may produce sub-optimal results.

Fluorophore	Excitation (nm)	Emission (nm)
AQUA	432	472
GREEN	498	521
ORANGE	546	575
RED	593	618

Limitations:

The optimum probe dilution and protocols for specific applications may vary. These include, but are not limited to; sample preparation, hybridization conditions and incubation times, post hybridization washes and microscope filter specifications and illumination conditions. The recommended hybridization times and wash conditions are for guidance only and it is the responsibility of the operator to determine optimal conditions. The clinical interpretation of any positive or negative hybridization events should be evaluated within the context of

 EMERGO EUROPE
Prinsessegracht 20
2514 AP The Hague
The Netherlands

Copy Control 15 Red FISH Probe

Control Number: 901-7217-071817

BIOCARE
M E D I C A L

clinical presentation, morphological and/or cytogenetic criteria by a suitably qualified practitioner. These findings should be complemented by the use of appropriate controls and other diagnostic tests where appropriate.

Quality Control:

Fluorescence In-Situ Hybridization (FISH) Methods for Clinical Laboratories; Approved Guidelines – Second edition (MM07-A2). CLSI, Wayne, PA (www.clsi.org). 2013.

Precautions:

1. This product contains formamide, which may be toxic. Formamide may cause serious eye damage or reproductive toxicity. It may also cause irritation by inhalation or skin contact. Avoid any direct contact exposure to reagent. Take appropriate protective measures (use disposable gloves, protective glasses, and lab garments).
2. Specimens, before and after fixation, and all materials exposed to them should be handled as if capable of transmitting infection and disposed of with proper precautions. Never pipette reagents by mouth and avoid contacting the skin and mucous membranes with reagents and specimens. If reagents or specimens come in contact with sensitive areas, wash with copious amounts of water¹.
3. The SDS is available upon request and is located at <http://biocare.net>.

Troubleshooting:

Follow the FISH probe specific protocol recommendations according to data sheet provided. If atypical results occur, contact Biocare Medical's Technical Support at 1-800-542-2002.

References:

1. Clinical and Laboratory Standards Institute (CLSI). Protection of Laboratory workers from occupationally Acquired Infections; Approved Guideline-Fourth Edition CLSI document M29-A4 Wayne, PA 2014.



60 Berry Drive
Pacheco, CA 94553
USA



Rev: 062117

Tel: 800-799-9499 | www.biocare.net | Fax: 925-603-8080



Prinsessegracht 20
2514 AP The Hague
The Netherlands